


DIAL GAGE TESTER CODE 2396-25A

ATTENTION: NOT SUITABLE FOR GAGES WITH GRADUATION 0.001MM



2396-25A

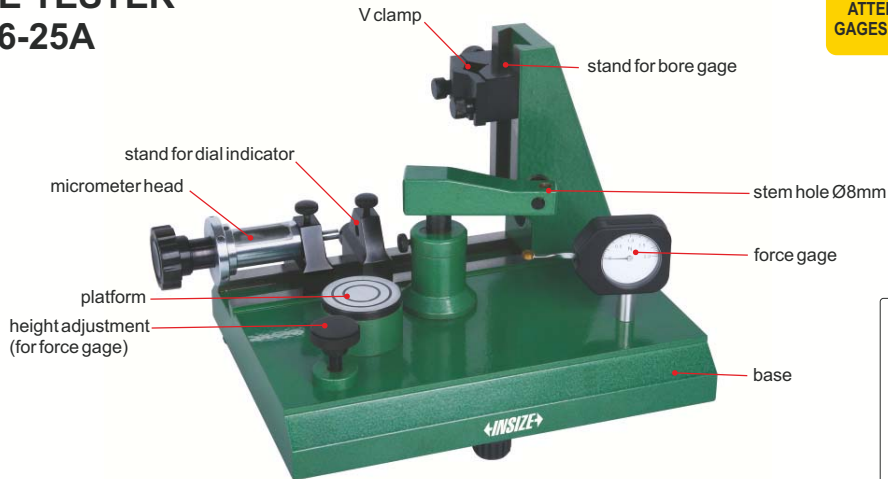

Micrometer head

Range	Sampling interval	Accuracy	Hysteresis
0-25mm	0.1mm	4µm(0-25mm), 3µm(0-10mm), 2µm(0-1mm)	1µm

Force gage

Range	Graduation	Accuracy
0-1.6N	0.05N	±5%(of load capacity)

Platform

Diameter	Flatness	Roughness
50mm	1µm	0.05µm

Half round gage block(optional)

Code	Parallelism
2396-block	1µm

- To calibrate dial indicators, test indicators and dial bore gages
- Dimension: 270x210x205mm
- Weight: 11kg



Inspect accuracy of dial indicators(range 0-25mm)



Inspect accuracy of dial bore gages (range 6-450mm)



Inspect accuracy of test indicators



Test force of dial indicators



Test repeatability of dial indicators



Test the effect of lateral force on accuracy of dial indicators (half round gage block is required)



Test the effect of lateral force on accuracy of test indicators (half round gage block is required)